



# Assessment form

Name: \_\_\_\_\_ Date of Birth: \_\_\_\_\_

Which incontinence product is used during the assesment:

Day and evening use:

Night use:



Time of incontinence product change	Number of areas that have changed colour	Wet clothes or bed		Faecel soiled		Supportive toilet visitation		Urination / bowel movements during toilet visits		Type of new incontinence product applied	Initials
		Yes	No	Yes	No	Yes	No	Yes U: urine / B: bowel	No		
Day 1 Date:	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									

Time of incontinence product change	Number of areas that have changed colour	Wet clothes or bed		Faecel soiled		Supportive toilet visitation		Urination / bowel movements during toilet visits		Type of new incontinence product applied	Initials
		Yes	No	Yes	No	Yes	No	Yes U: urine / B: bowel	No		
Day 1 Date:	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									

Time of incontinence product change	Number of areas that have changed colour	Wet clothes or bed		Faecel soiled		Supportive toilet visitation		Urination / bowel movements during toilet visits		Type of new incontinence product applied	Initials
		Yes	No	Yes	No	Yes	No	Yes U: urine / B: bowel	No		
Day 3 Date:	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									
	At	Areas									

## Wetness indicator with graduation scale

- The wetness indicator consists of two yellow lines printed on the backsheet foil. The two yellow lines turn blue when it gets wet, giving an indication when the pad needs to be changed.
- Wetness indicator with graduation scale allows the caregiver to see how much of the product's capacity has been utilized.
- It guides the caregiver and the user to the product with the right absorption level complying with our overall objective: "As small as possible, as large as necessary."

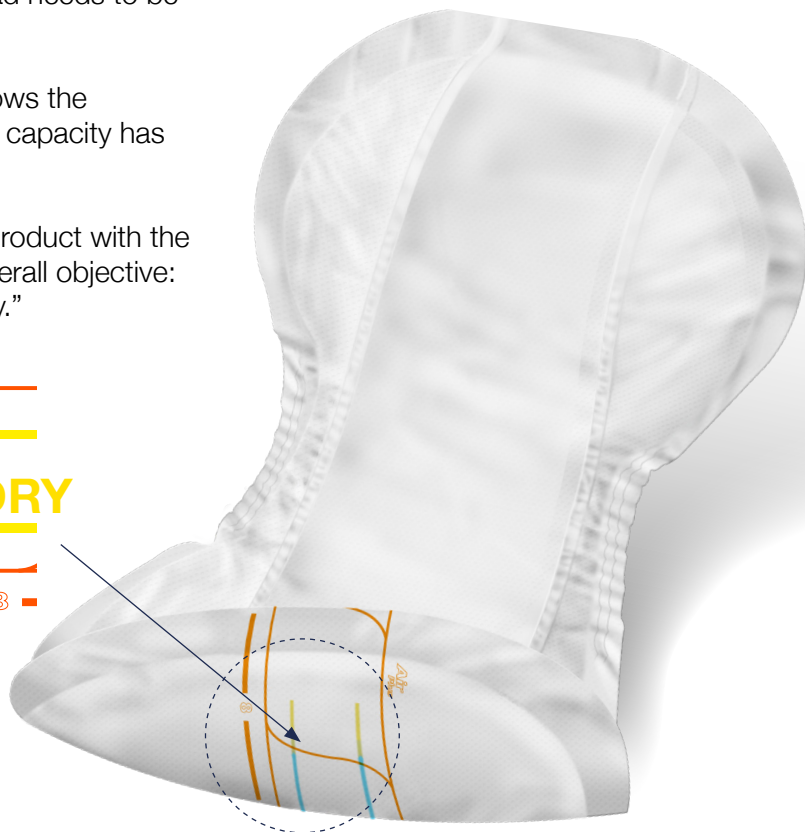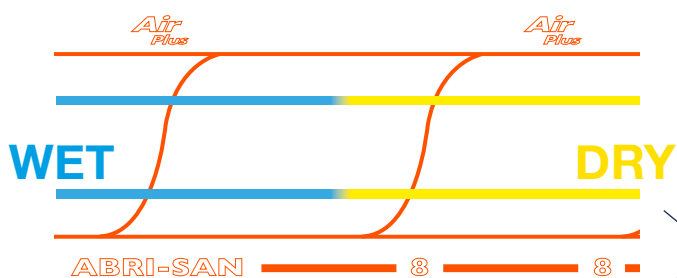

Below you can see how many areas each incontinence product has. This is used when using the wetness indicator as a professional tool for analyzing the product's utilization rate. For instance, if only three out of seven areas of a product have changed colours, this shows that the absorption level of the product is too high in relation to the need. In general, the product is fully utilized when 75% of the areas have changed colour.

### Graduation areas

Shaped pad <b>Abri-San</b>	Pants <b>Abri-Flex</b>	All-in-one brief <b>Abri-Form</b>	Belted product <b>Abri-Wing</b>
<b>5:</b> Totally 8 areas	<b>Junior XS2:</b> Totally 4 areas	<b>XS:</b> Totally 6 areas	<b>S:</b> Totally 7 areas
<b>6:</b> Totally 8 areas	<b>XS:</b> None	<b>S:</b> Totally 8 areas	<b>M:</b> Totally 8 areas
<b>7:</b> Totally 8 areas	<b>S:</b> Totally 7 areas	<b>M:</b> Totally 9 areas	<b>L:</b> Totally 9 areas
<b>8:</b> Totally 8 areas	<b>M:</b> Totally 7 areas	<b>L:</b> Totally 11 areas	<b>XL:</b> Totally 10 areas
<b>9:</b> Totally 9 areas	<b>L:</b> Totally 8 areas	<b>XL:</b> Totally 11 areas	
<b>10:</b> Totally 9 areas	<b>XL:</b> Totally 8 areas		
<b>11:</b> Totally 9 areas			
<b>Special:</b> None			
<b>Abri-Man</b>			
<b>Special:</b> Totally 9 areas			